


# AIRE~IVF™ SYSTEM CLINICAL OUTCOME DATA


## Aire~IVF™

The Aire-IVF™ System is a revolutionary air purification solution designed to irradiate and inactivate biologicals, eliminate embryotoxic VOCs, and significantly reduce particulates.

### CLINICAL PREGNANCY RATES

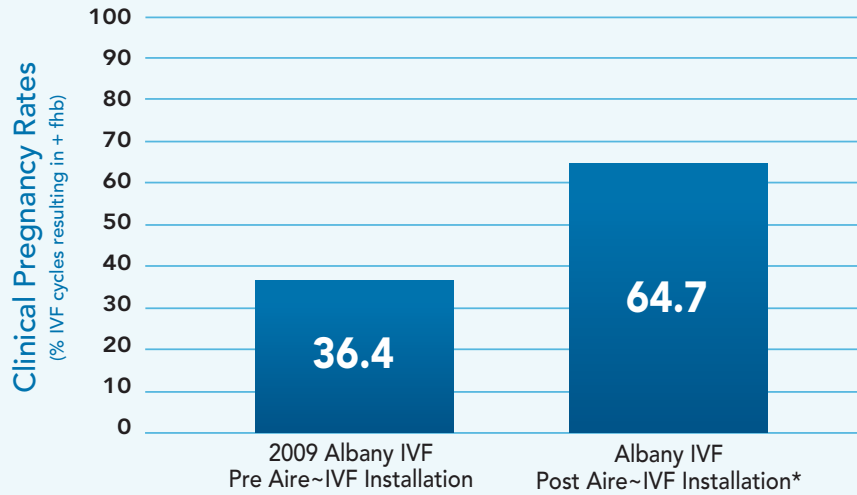

### IMPLANTATION RATES

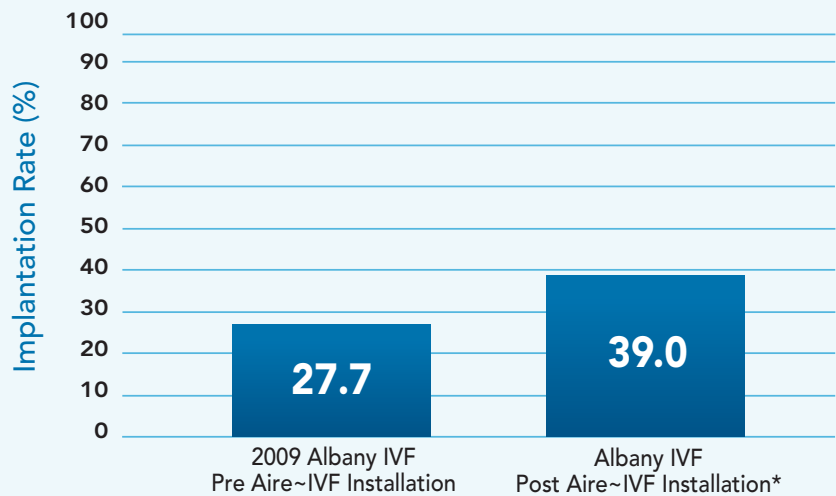

\*ongoing data

### National Homeland Security Research Center

The UV output/intensity in Aire~IVF™ was validated in its "kill or inactivation" rate towards:

- Airborne bacteria: >99.97% (*Serratia marcescens*)
- Airborne viral: 99.00% (MS2 virus)
- Anthrax surrogate: 93.00% (*Bacillus atrophaeus*)
- Biological warfare agents: 99.97%

### Third Party Independent Testing

	Source Air	IVF Laboratory using Aire~IVF
TVOC	1400 ppb	Below detection limits of <5 ppb
Biologicals: Spores	>15,240/M <sup>3</sup>	Below detection limits of <1/M <sup>3</sup>
Particulates	>1,063,435 0.3 um particulates	5,410 0.3 um particulates

Based upon 2009 data as reported to SART. This data has not been verified by the CDC. A message from SART, "As entry criteria are highly variable for each program, and treatment processes vary, a center by center comparison of results may not be meaningful." Patient characteristics vary among programs: results not guaranteed.



1275 Glenlivet Drive, Suite 100, Allentown, PA 18106-3107 • Phone 484-224-3042 • Fax 484-224-2999

[www.lifeaire.com](http://www.lifeaire.com)